


CLINICAL+ SUMMARY

STUDY CONFIRMS: **Families prefer MiniONE® over Mic-Key®¹**

In a recent single center prospective, randomized trial with a crossover design, Abdelhadi, et al. examined differences between the two most commonly used low-profile gastrostomy tubes (g-tubes): the MiniONE® (Applied Medical Technology Inc., Brecksville, OH) and the Mic-Key® (Avanos Medical Inc., Alpharetta, GA).¹

THE RESULTS ARE CLEAR:

Over 70% of families prefer the AMT MiniONE® over the Avanos Mic-Key®¹

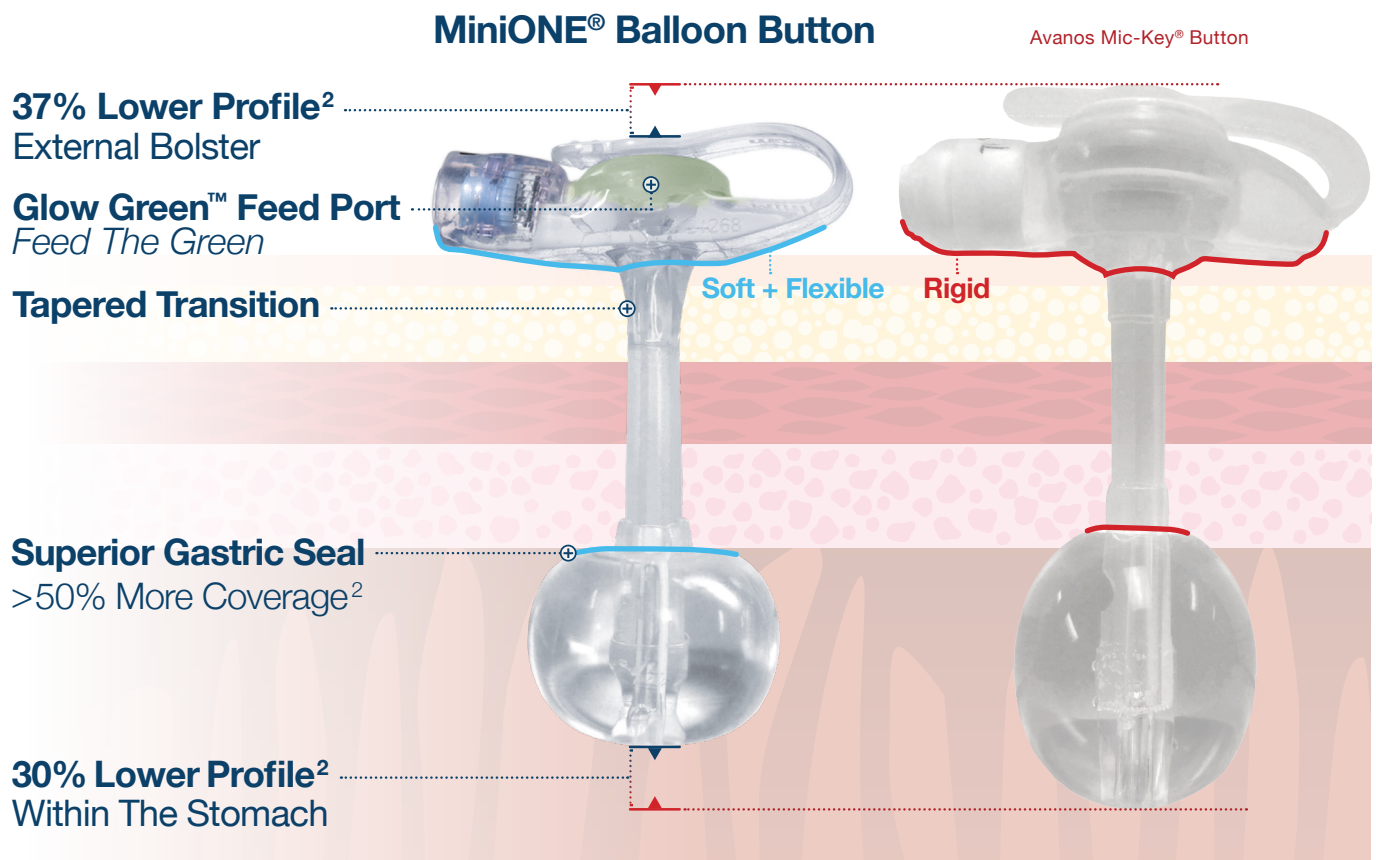

Families who preferred the MiniONE® stated they liked “the smaller size of the external bolster, the fact that it glows in the dark, and that it seemed to cause less skin problems and be less likely to snag or accidentally get dislodged.”¹

Patient, family, and caregiver preference are important factors to consider when selecting a low-profile g-tube because management of home enteral nutrition requires significant participation and commitment.¹



Innovating. Educating. Changing Lives.™


AMT MiniONE® Balloon Button



Exclusive AMT Balloon
Superior Gastric Seal



Soft + Flexible
Optimized for Comfort

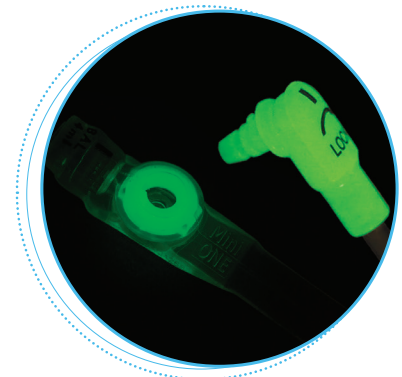

Glow Green™
Easier Nighttime Feeds

An Advantage In Enteral Nutrition

AMT®	12F		14F		16F		18F		20F		24F	
Length CM	ORDER NUMBERS											
	LEGACY	ENFit®	LEGACY	ENFit®	LEGACY	ENFit®	LEGACY	ENFit®	LEGACY	ENFit®	LEGACY	ENFit®
0.8	M1-5-1208	M1-5-1208-I	M1-5-1408	M1-5-1408-I								
1.0	M1-5-1210	M1-5-1210-I	M1-5-1410	M1-5-1410-I	M1-5-1610	M1-5-1610-I	M1-5-1810	M1-5-1810-I	M1-5-2010	M1-5-2010-I		
1.2	M1-5-1212	M1-5-1212-I	M1-5-1412	M1-5-1412-I	M1-5-1612	M1-5-1612-I	M1-5-1812	M1-5-1812-I	M1-5-2012	M1-5-2012-I		
1.5	M1-5-1215	M1-5-1215-I	M1-5-1415	M1-5-1415-I	M1-5-1615	M1-5-1615-I	M1-5-1815	M1-5-1815-I	M1-5-2015	M1-5-2015-I	M1-5-2415	M1-5-2415-I
1.7	M1-5-1217	M1-5-1217-I	M1-5-1417	M1-5-1417-I	M1-5-1617	M1-5-1617-I	M1-5-1817	M1-5-1817-I	M1-5-2017	M1-5-2017-I	M1-5-2417	M1-5-2417-I
2.0	M1-5-1220	M1-5-1220-I	M1-5-1420	M1-5-1420-I	M1-5-1620	M1-5-1620-I	M1-5-1820	M1-5-1820-I	M1-5-2020	M1-5-2020-I	M1-5-2420	M1-5-2420-I
2.3	M1-5-1223	M1-5-1223-I	M1-5-1423	M1-5-1423-I	M1-5-1623	M1-5-1623-I	M1-5-1823	M1-5-1823-I	M1-5-2023	M1-5-2023-I	M1-5-2423	M1-5-2423-I
2.5	M1-5-1225	M1-5-1225-I	M1-5-1425	M1-5-1425-I	M1-5-1625	M1-5-1625-I	M1-5-1825	M1-5-1825-I	M1-5-2025	M1-5-2025-I	M1-5-2425	M1-5-2425-I
2.7	M1-5-1227	M1-5-1227-I	M1-5-1427	M1-5-1427-I	M1-5-1627	M1-5-1627-I	M1-5-1827	M1-5-1827-I	M1-5-2027	M1-5-2027-I	M1-5-2427	M1-5-2427-I
3.0	M1-5-1230	M1-5-1230-I	M1-5-1430	M1-5-1430-I	M1-5-1630	M1-5-1630-I	M1-5-1830	M1-5-1830-I	M1-5-2030	M1-5-2030-I	M1-5-2430	M1-5-2430-I
3.5	M1-5-1235	M1-5-1235-I	M1-5-1435	M1-5-1435-I	M1-5-1635	M1-5-1635-I	M1-5-1835	M1-5-1835-I	M1-5-2035	M1-5-2035-I	M1-5-2435	M1-5-2435-I
4.0	M1-5-1240	M1-5-1240-I	M1-5-1440	M1-5-1440-I	M1-5-1640	M1-5-1640-I	M1-5-1840	M1-5-1840-I	M1-5-2040	M1-5-2040-I	M1-5-2440	M1-5-2440-I
4.4			M1-5-1444	M1-5-1444-I	M1-5-1644	M1-5-1644-I	M1-5-1844	M1-5-1844-I	M1-5-2044	M1-5-2044-I	M1-5-2444	M1-5-2444-I
5.0			M1-5-1450	M1-5-1450-I	M1-5-1650	M1-5-1650-I	M1-5-1850	M1-5-1850-I	M1-5-2050	M1-5-2050-I	M1-5-2450	M1-5-2450-I
5.5			M1-5-1455	M1-5-1455-I	M1-5-1655	M1-5-1655-I	M1-5-1855	M1-5-1855-I	M1-5-2055	M1-5-2055-I	M1-5-2455	M1-5-2455-I
6.0			M1-5-1460	M1-5-1460-I	M1-5-1660	M1-5-1660-I	M1-5-1860	M1-5-1860-I	M1-5-2060	M1-5-2060-I	M1-5-2460	M1-5-2460-I
6.5			M1-5-1465	M1-5-1465-I								
7.0			M1-5-1470	M1-5-1470-I								
8.0			M1-5-1480	M1-5-1480-I								
9.0			M1-5-1490	M1-5-1490-I								
10.0			M1-5-14100	M1-5-14100-I								

*The MiniONE® Balloon Button comes packaged as 1/box.

1. Abdelhadi, Ruba A.; Dekonenko, Charlene; Dorman, Robert M., et al. A Prospective, Randomized Cross-over Trial of Two Low-profile Gastrostomy Buttons to Determine Family Preference. *JPGN* 2020;70:386 – 388.
https://journals.lww.com/jpgn/Abstract/2020/03000/A_Prospective_Randomized_Cross_over_Trial_of_2.25.aspx

2. Claims based on internal testing of 14F devices.

Full-Text Article:



For a complete list of products visit us at www.AppliedMedical.net
800 869 7382 | CS@AppliedMedical.net | ICS@AppliedMedical.net



MiniONE® Balloon Button



Applied Medical Technology, Inc.
8006 Katherine Boulevard
Brecksville, OH 44141
www.AppliedMedical.net
An ISO 13485 Registered Company
MR Conditional
Made In USA



© 2022 Applied Medical Technology, Inc. C-4708-D

Patents: <http://www.AppliedMedical.net/Patents/> | Trademarks: <http://www.AppliedMedical.net/Trademarks/>
Mic-Key® is a registered trademark of Avent, Inc. | ENFit® is a registered trademark of GEDSA.